

Figure 1B

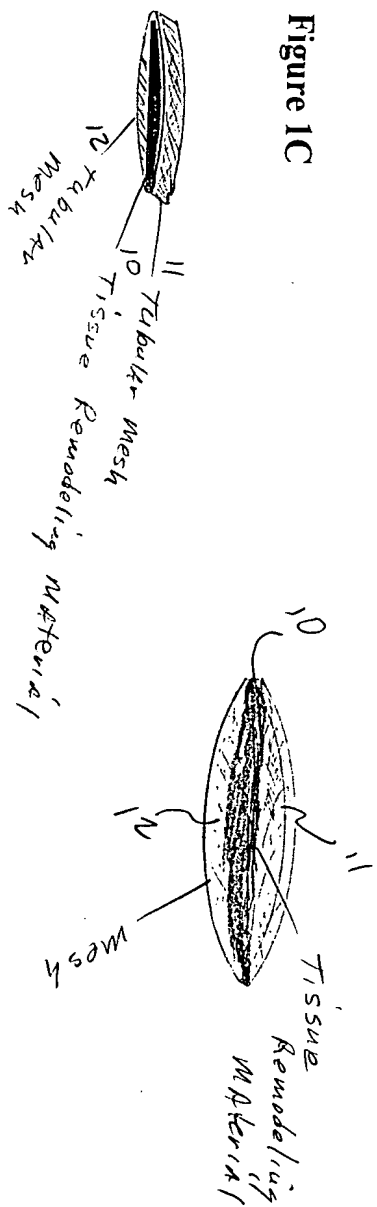


Figure 1C

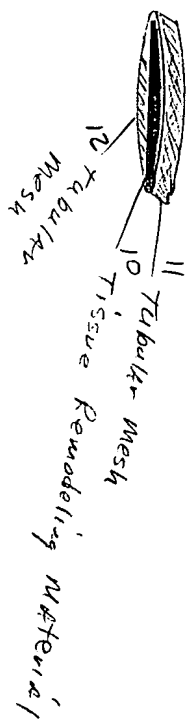


Figure 1

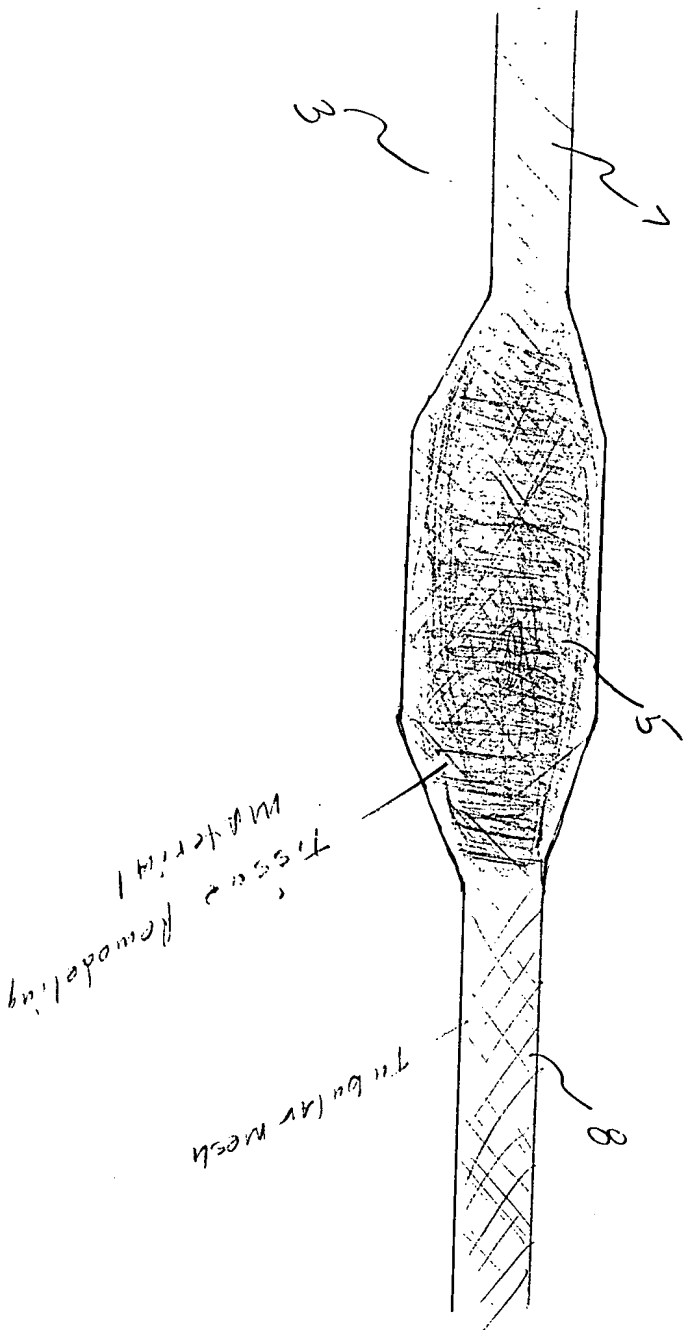


Figure 2A

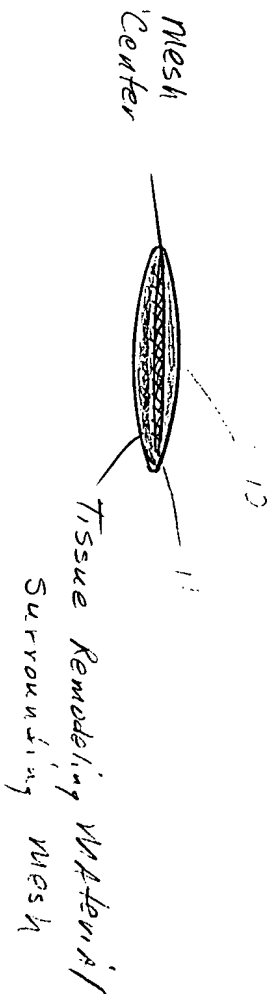
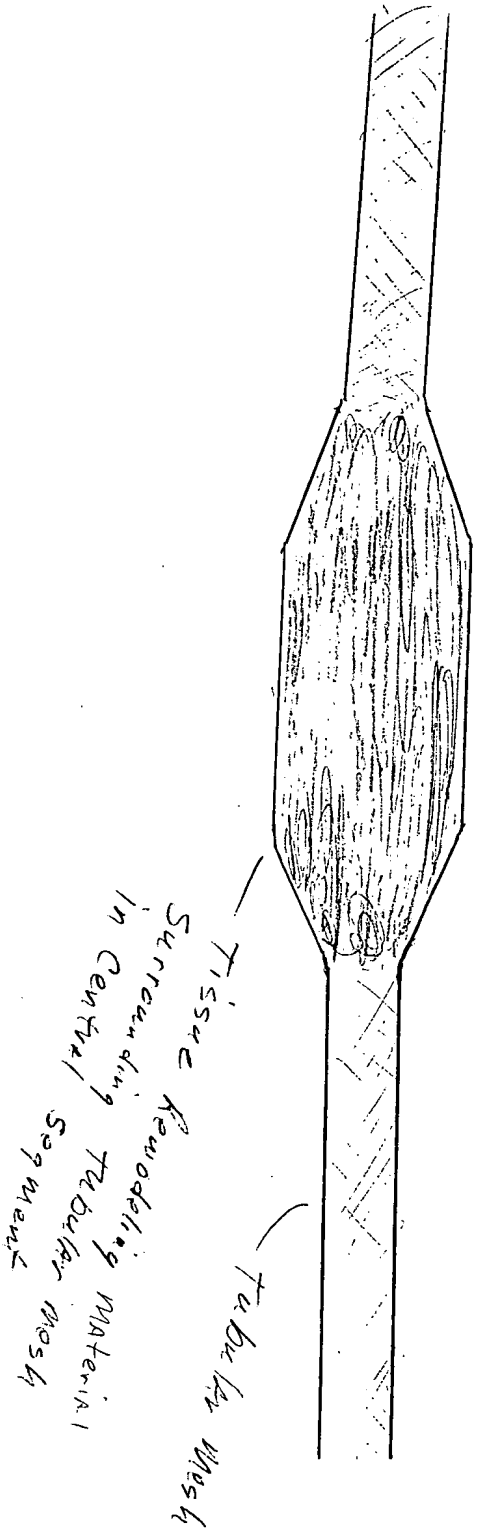
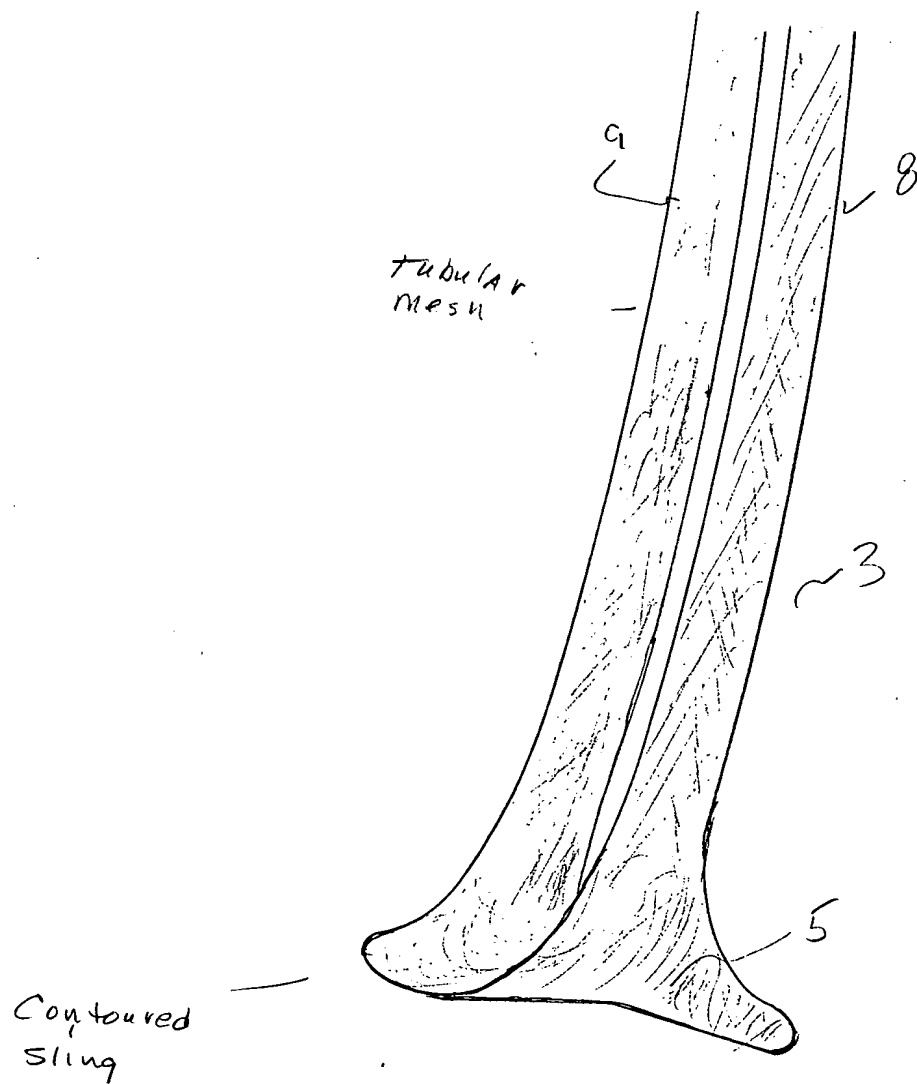
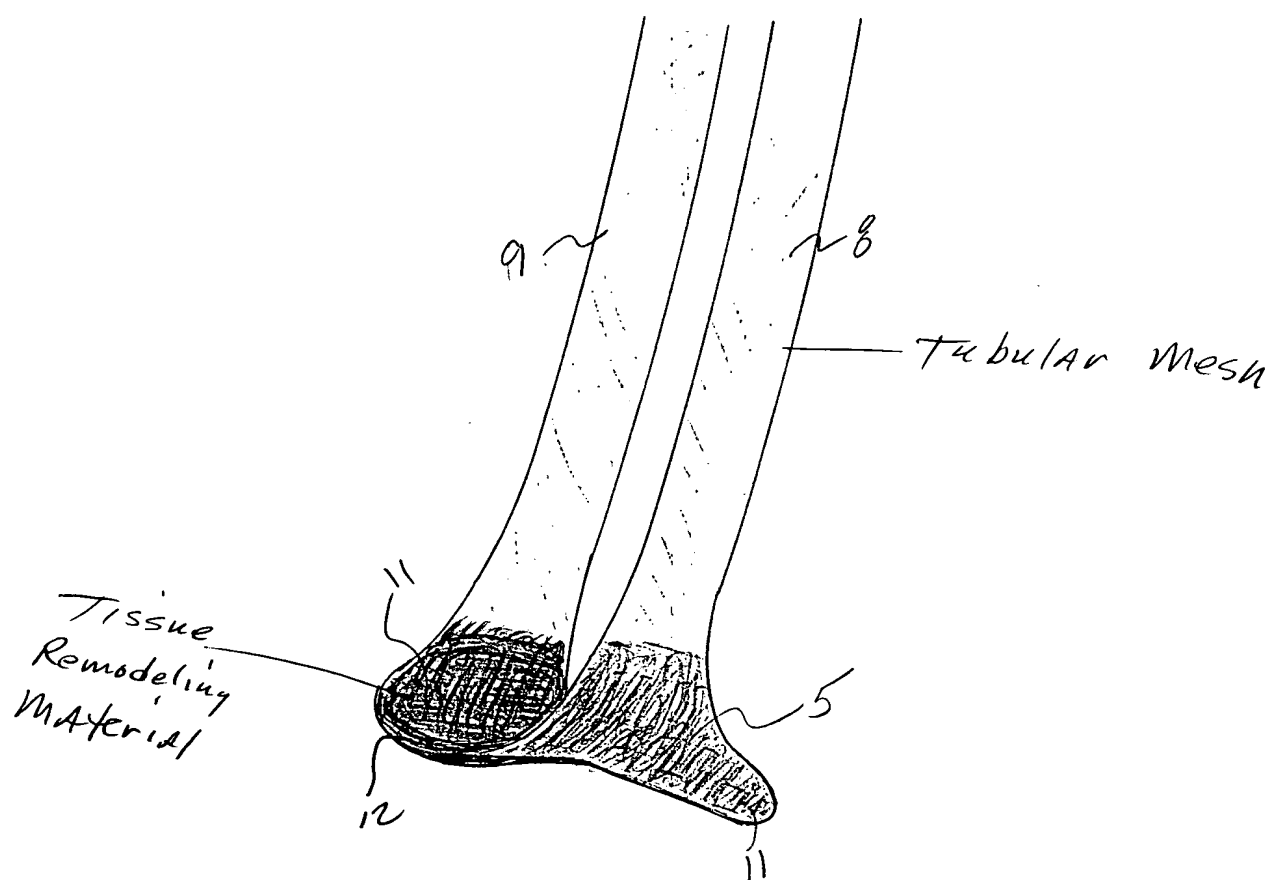


Figure 2





**Figure 3**



**Figure 3A**

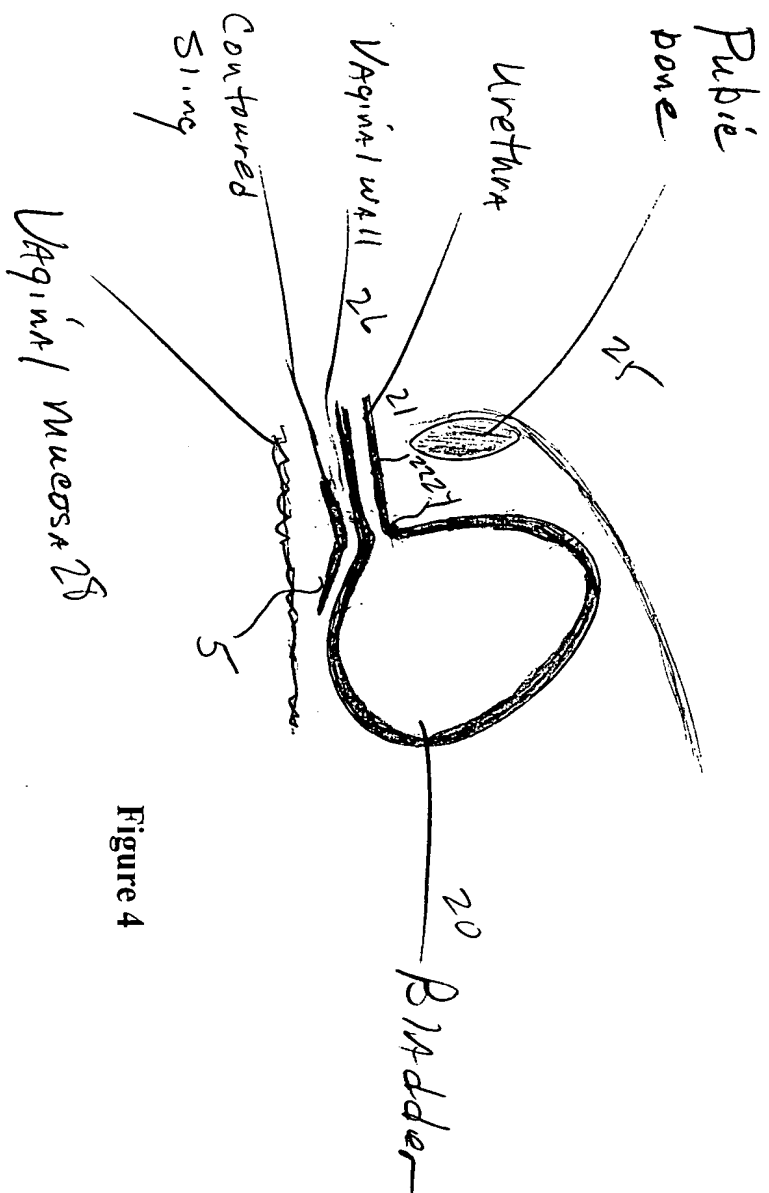


Figure 4

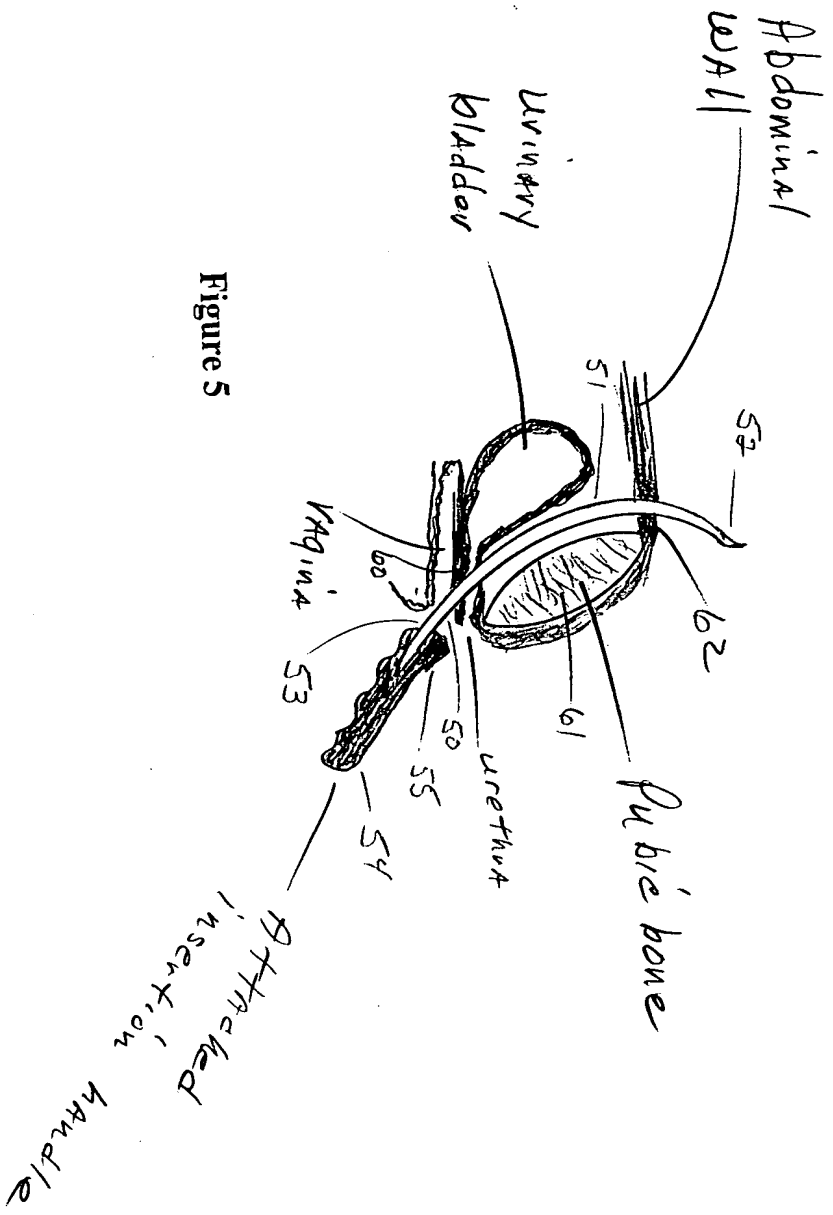


Figure 5

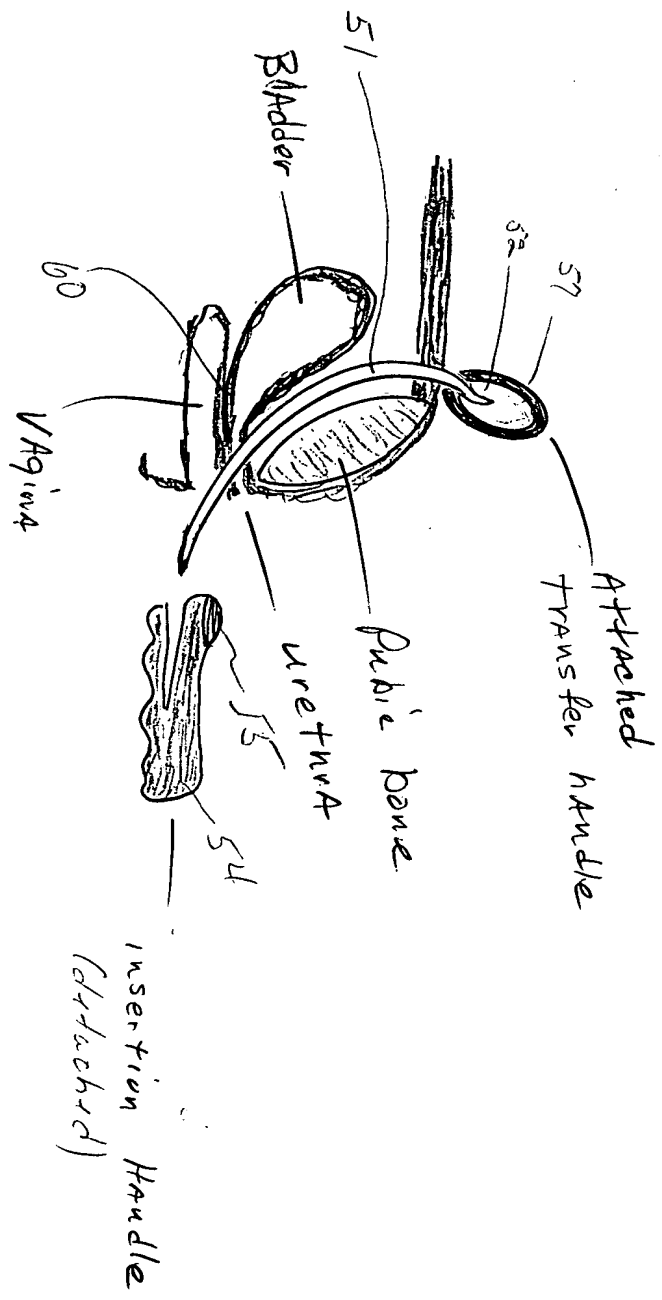


Figure 5A

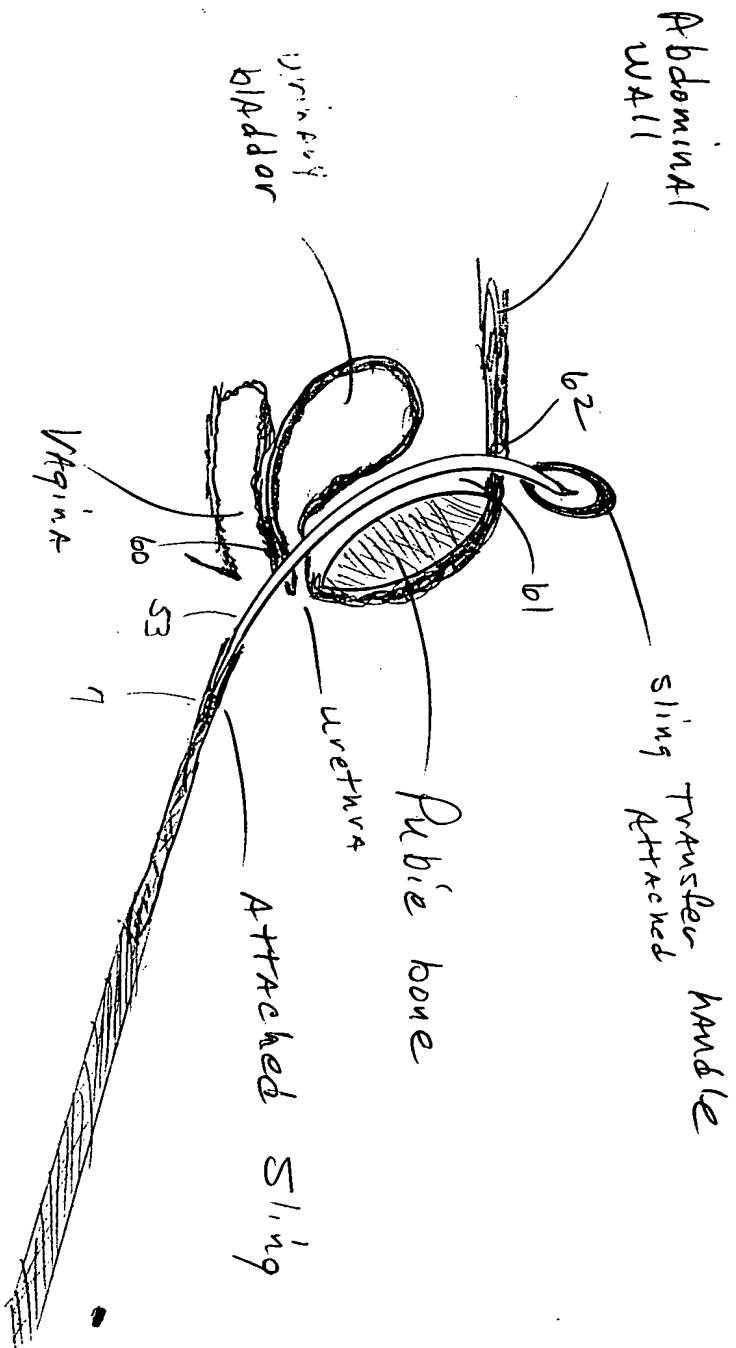


Figure 5B



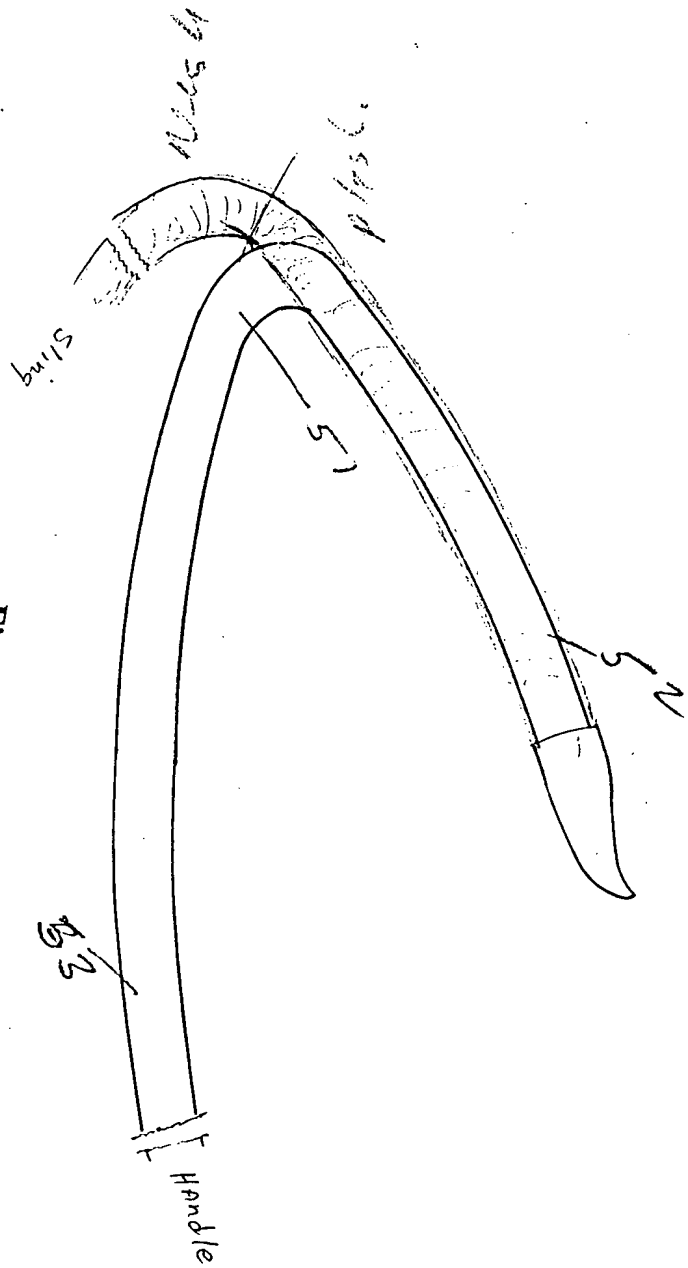


Figure 6

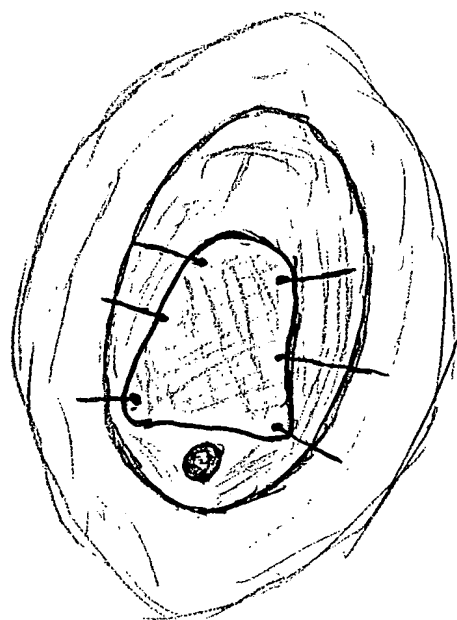


Figure 7

FORCED TO  
 WITHDRAW WHILE  
 SUPPORT DEVICES  
 WERE IN PLACE

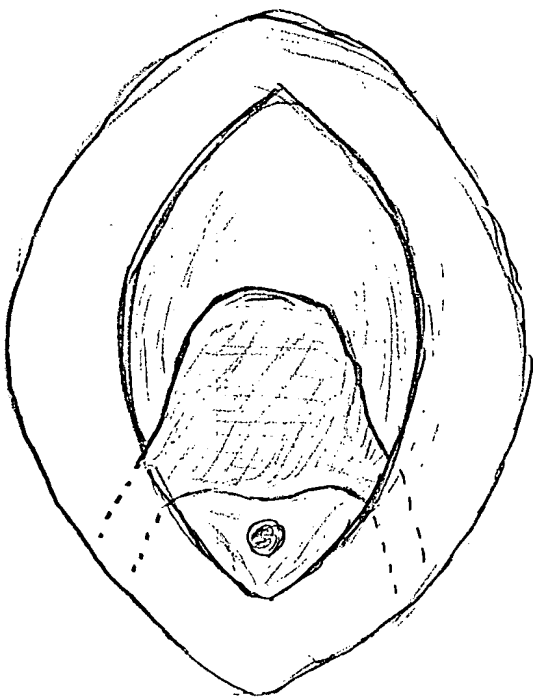


Figure 8

Handwritten notes, possibly describing the structure or process shown in the diagram.


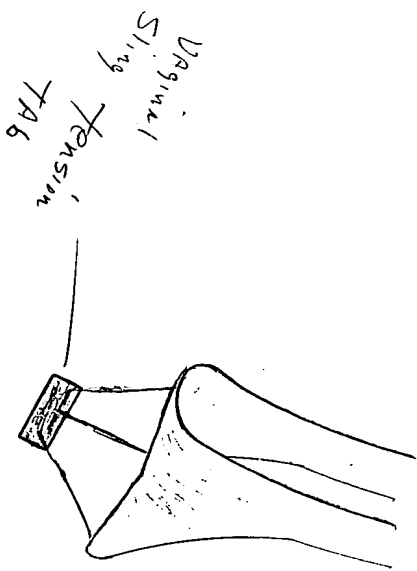




Figure 9

Sling tension  
Adjustment handle



Sling tension  
Adjustment handle to  
increase tension  
Postoperatively

Plastic hinge



Irregular inside  
surface for grasping  
the distal segment  
of the sling

Figure 10